



1/19

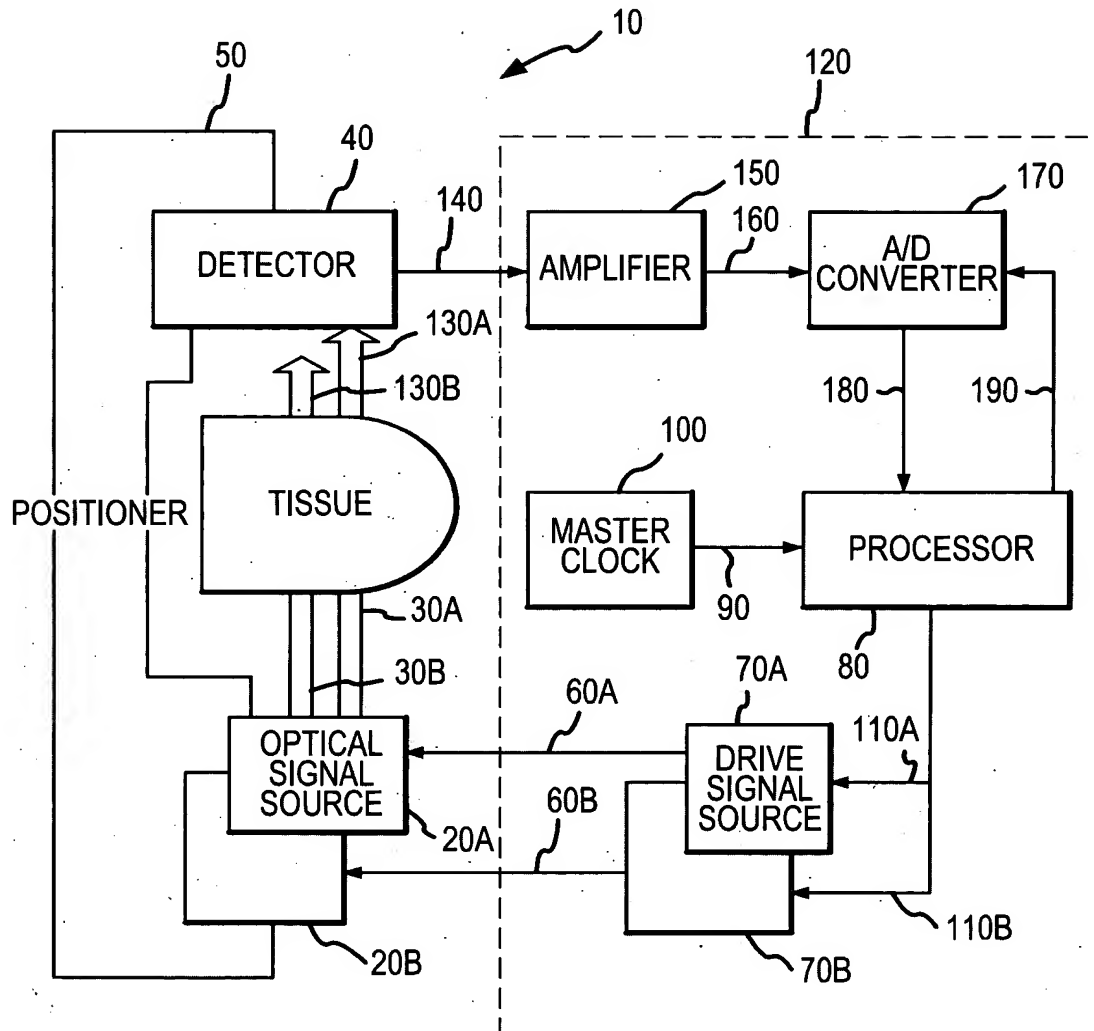


FIG.1

2/19

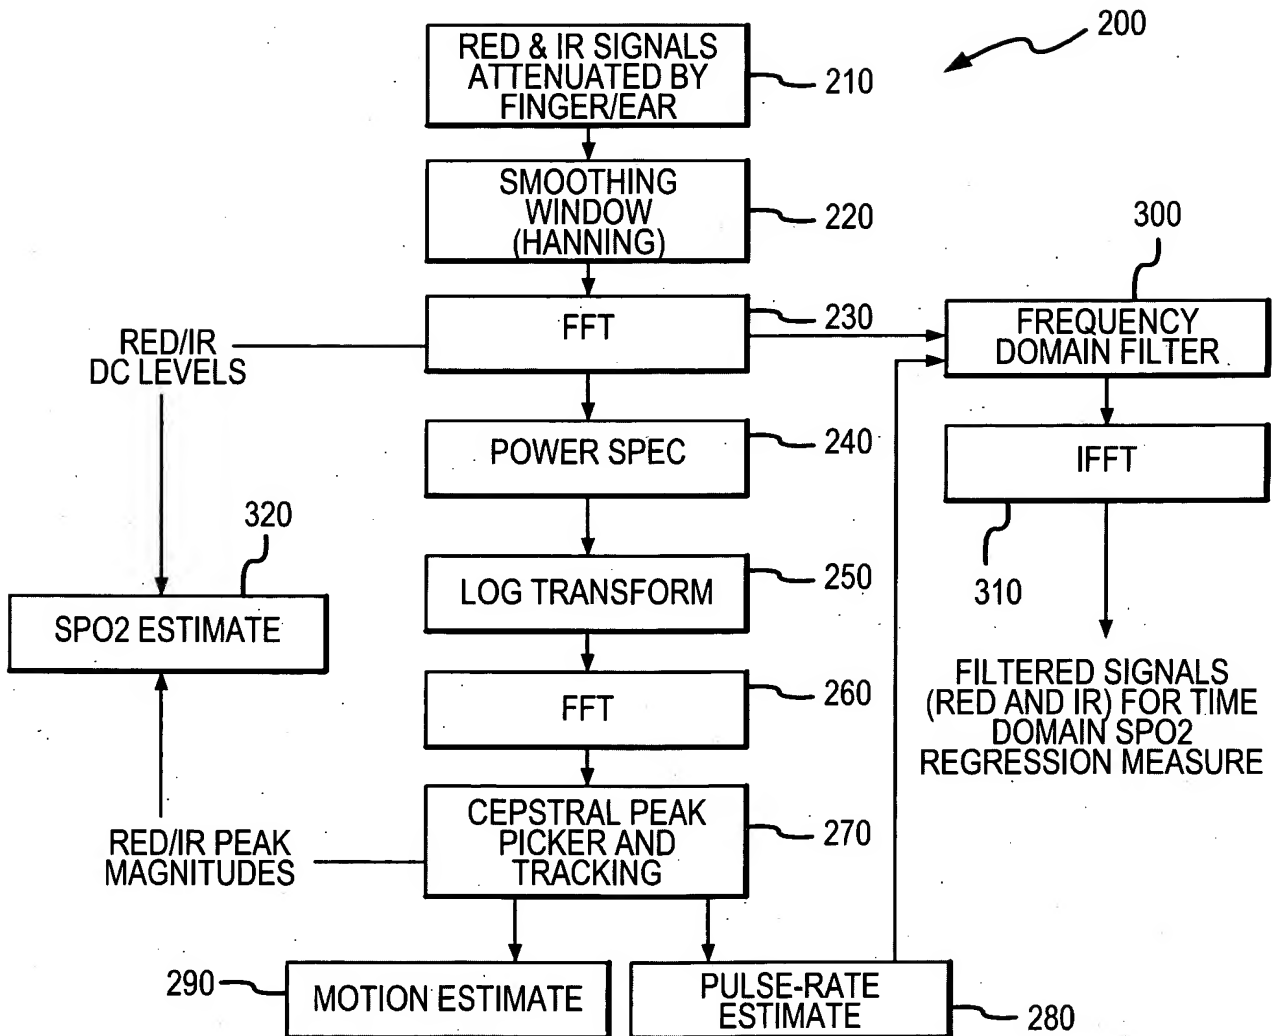


FIG.2

3/19

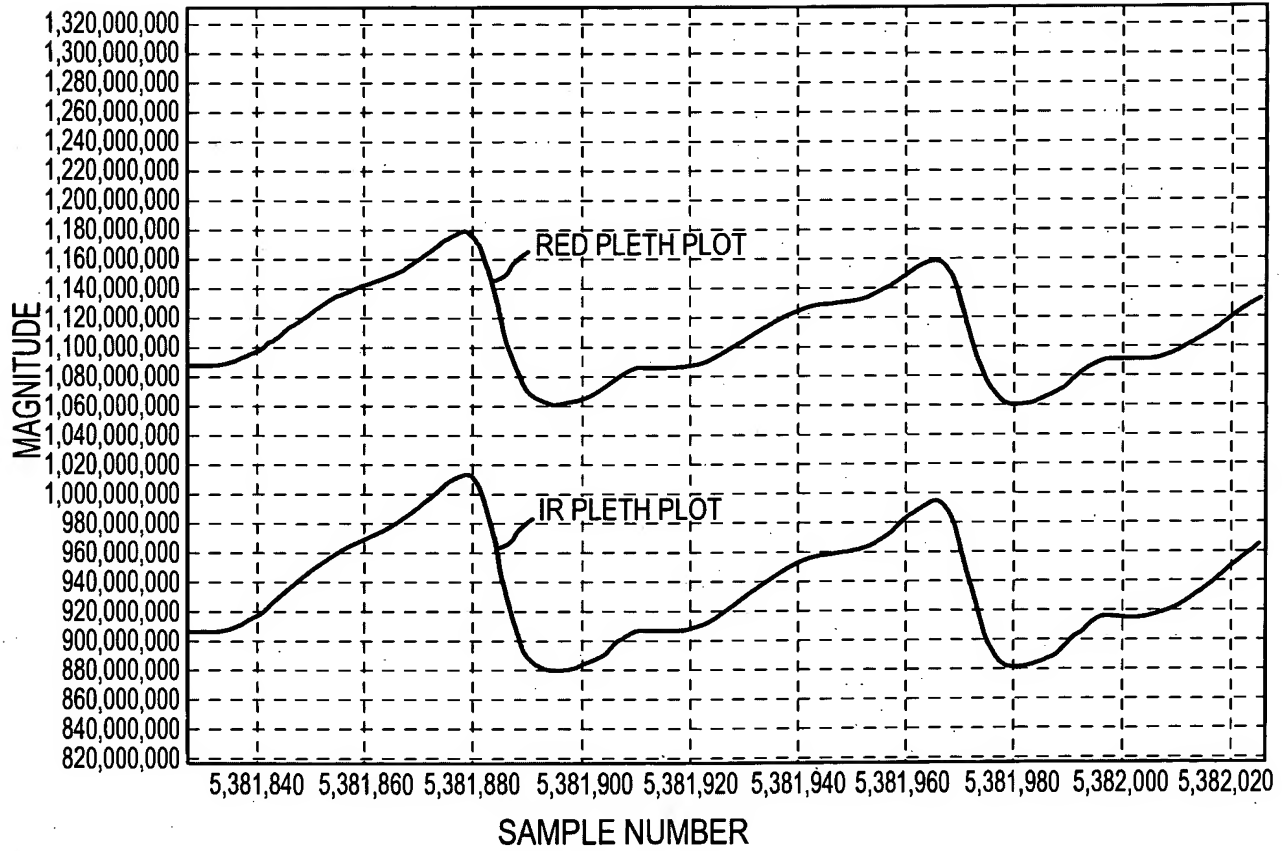


FIG.3A

4/19

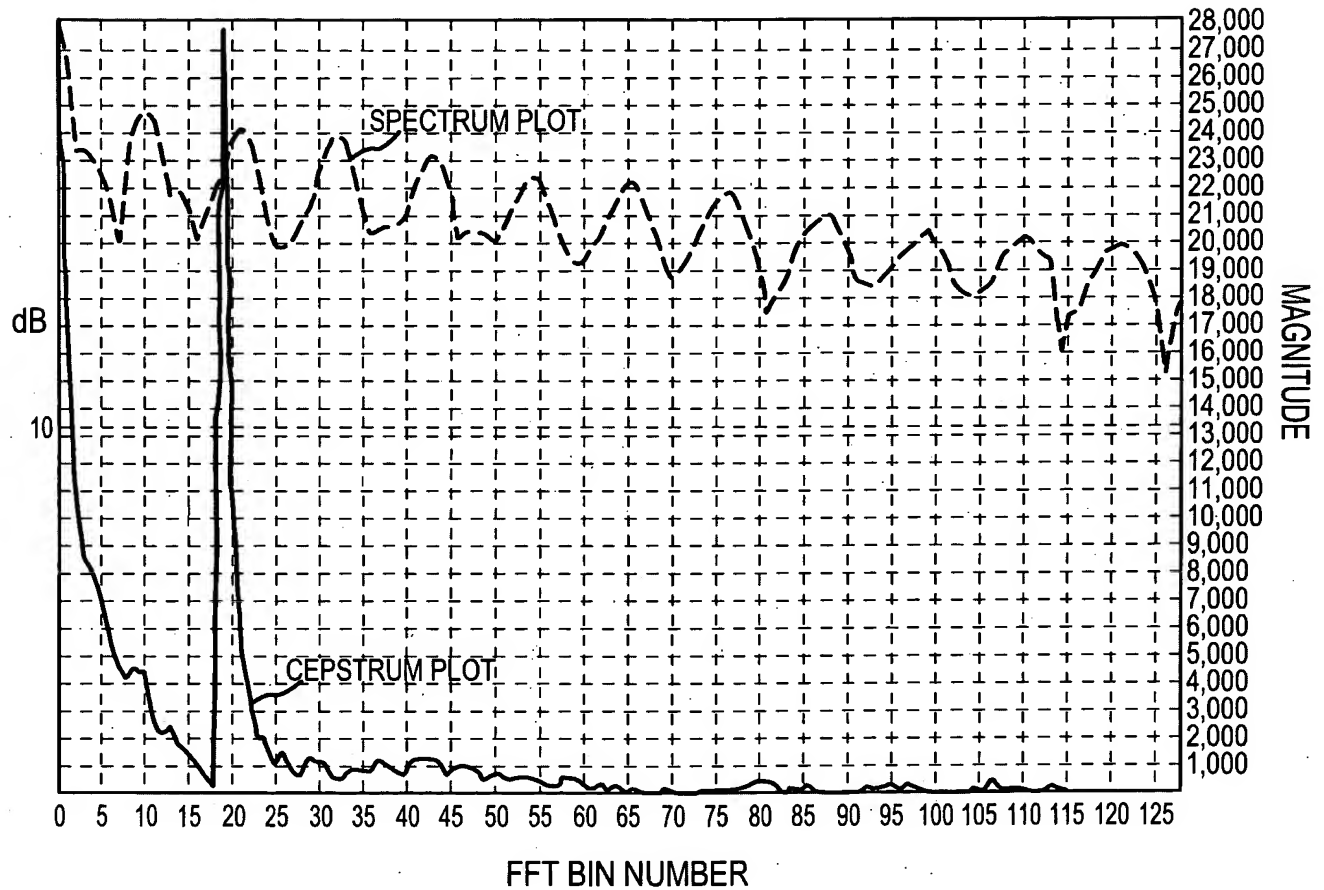


FIG.3B

5/19

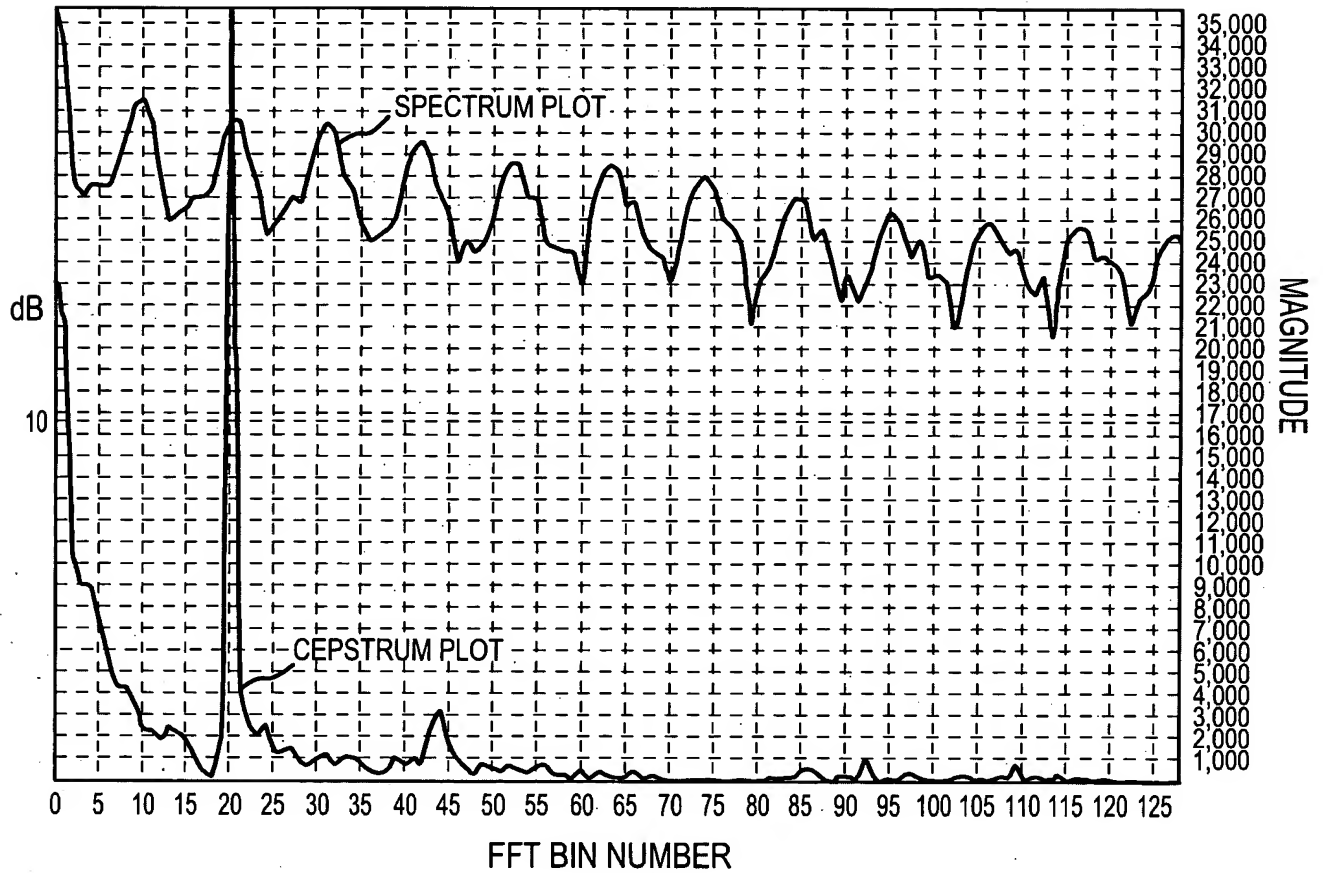


FIG.3C

6/19

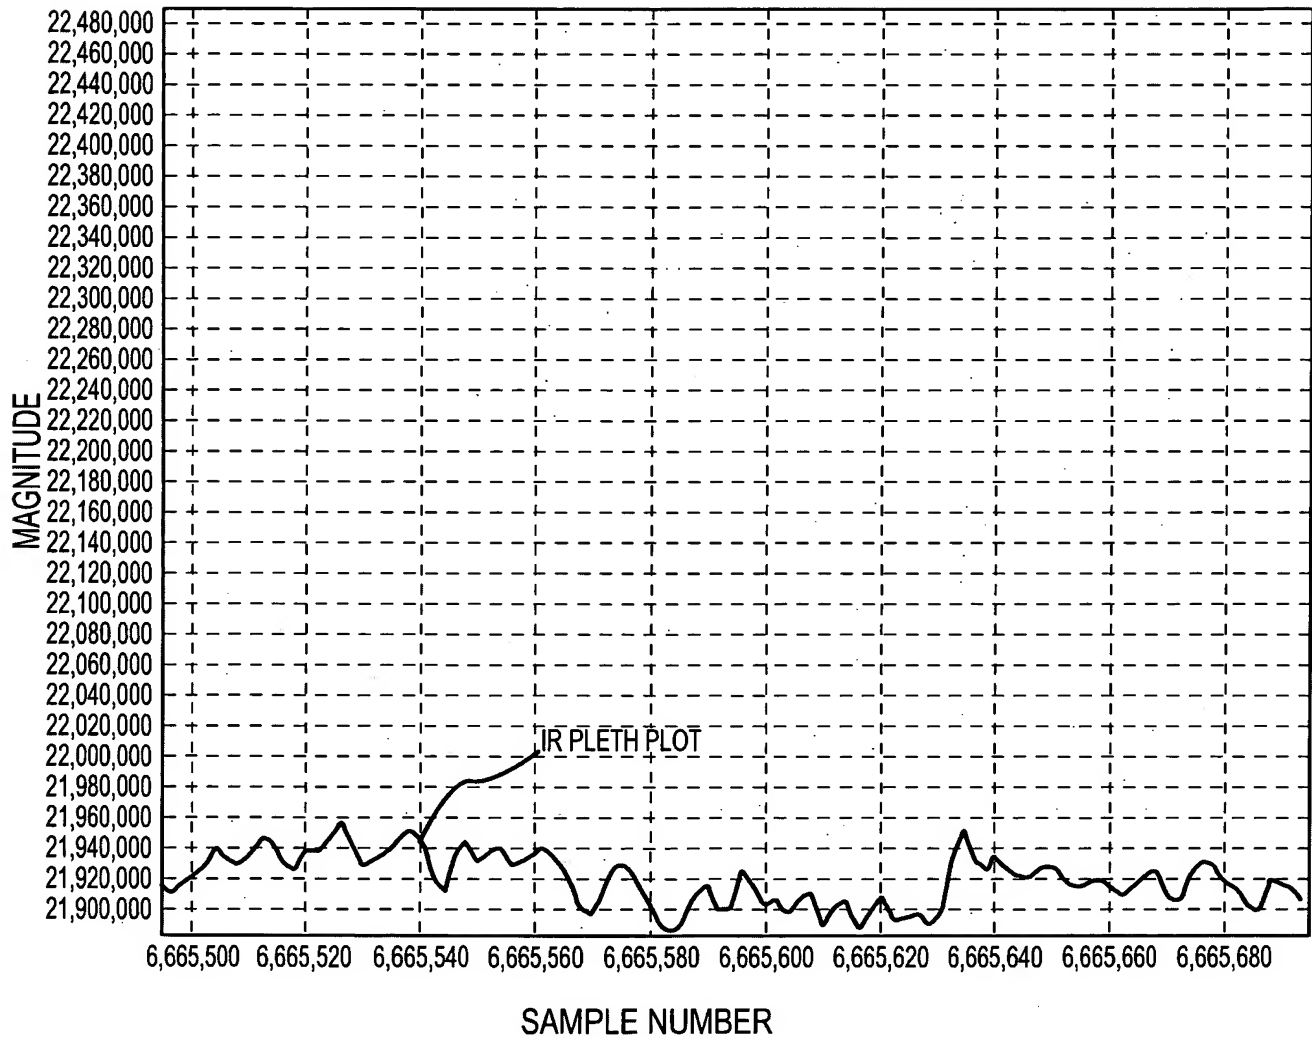


FIG.3D

7/19

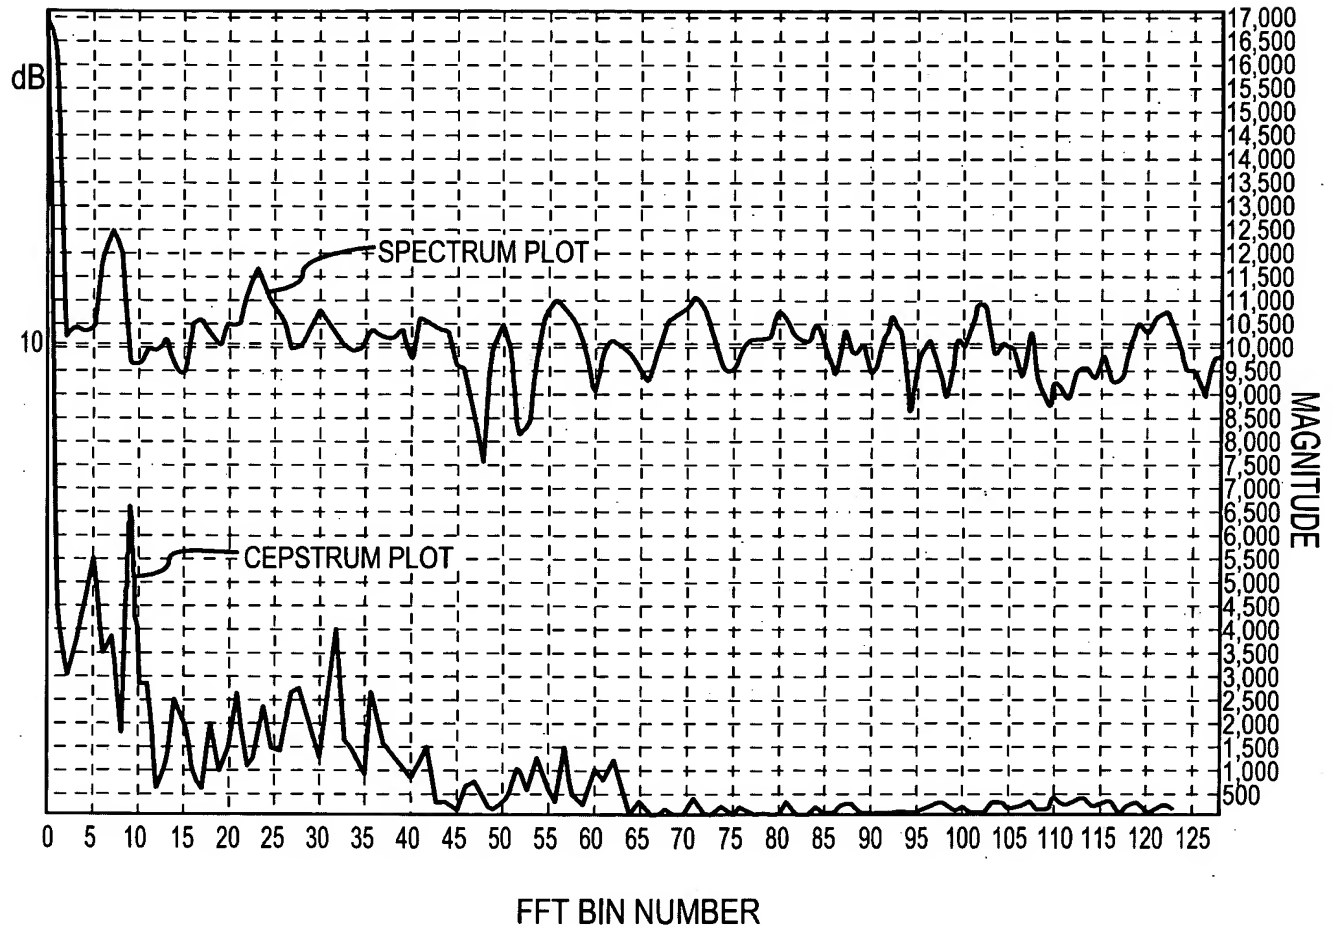


FIG.3E

8/19


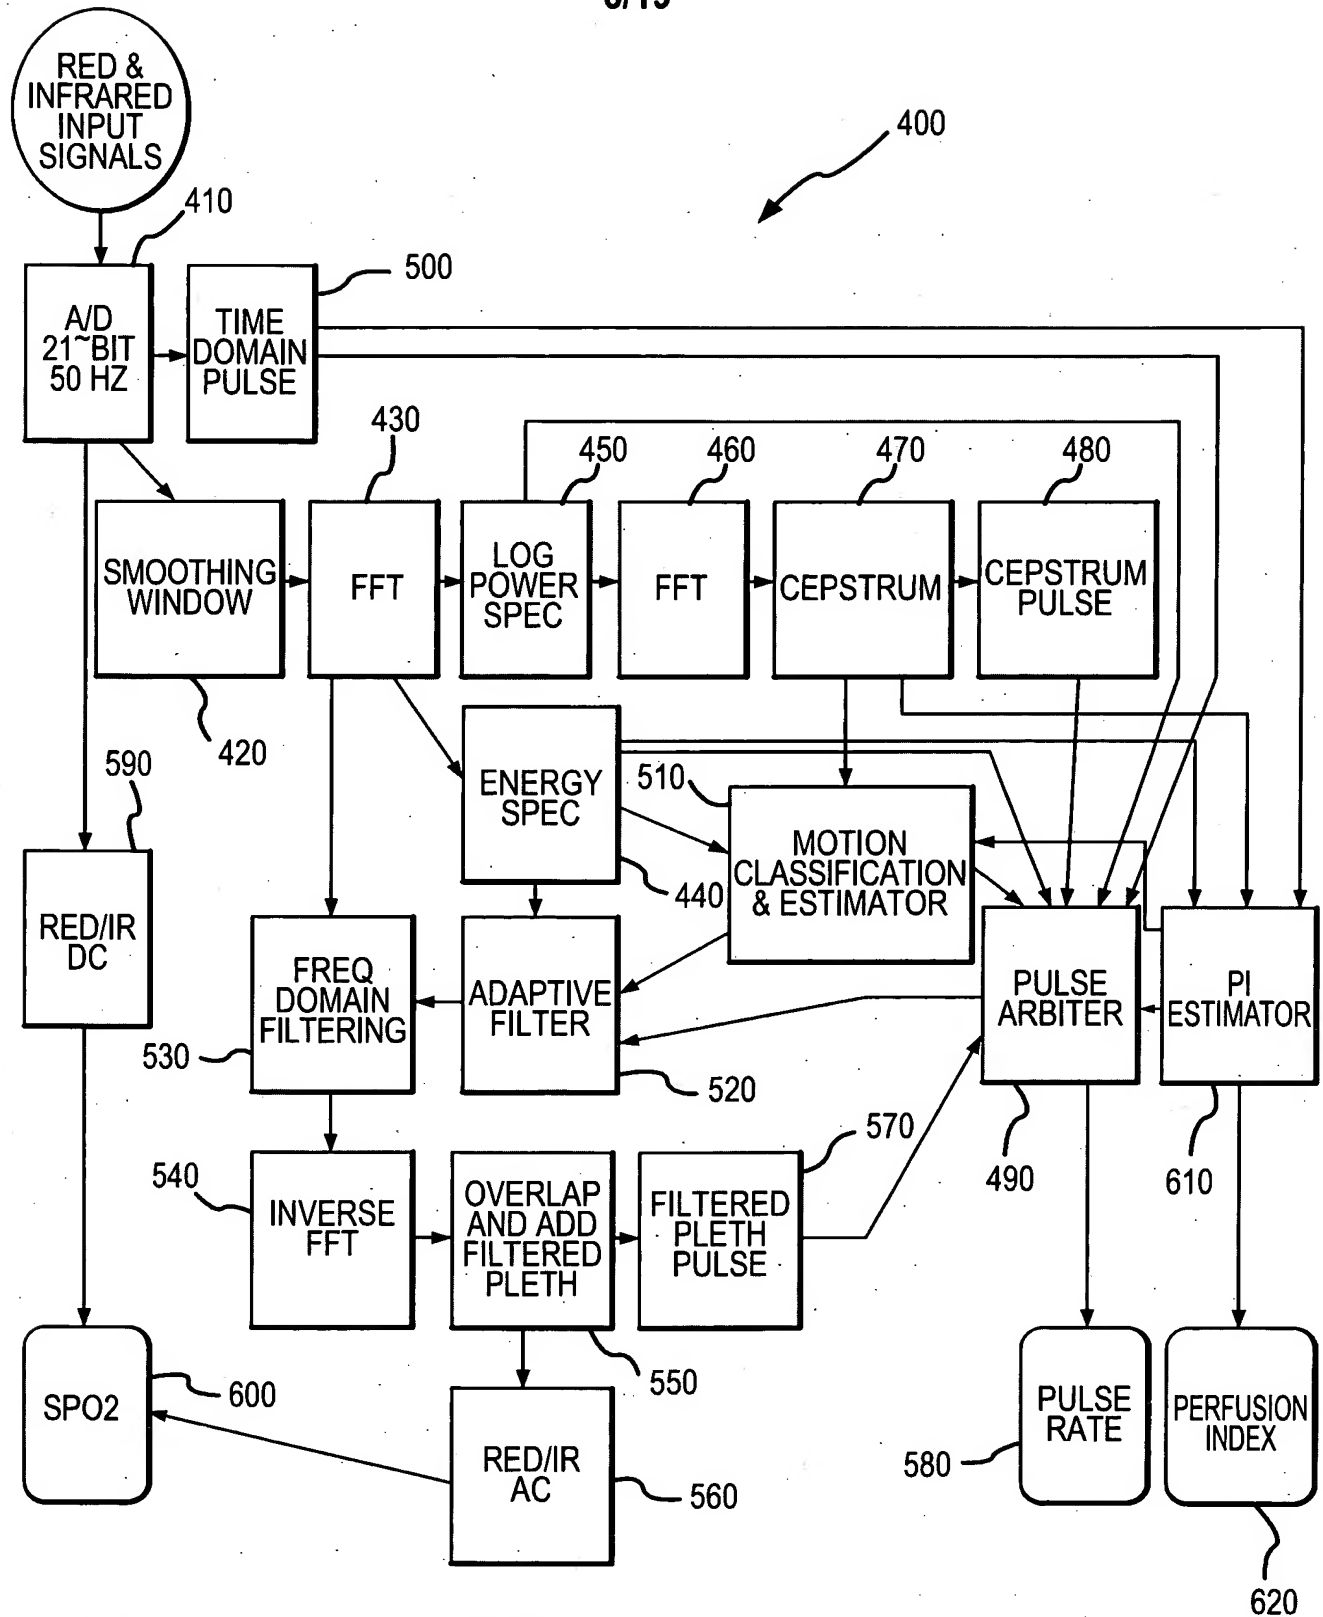



FIG.4

9/19

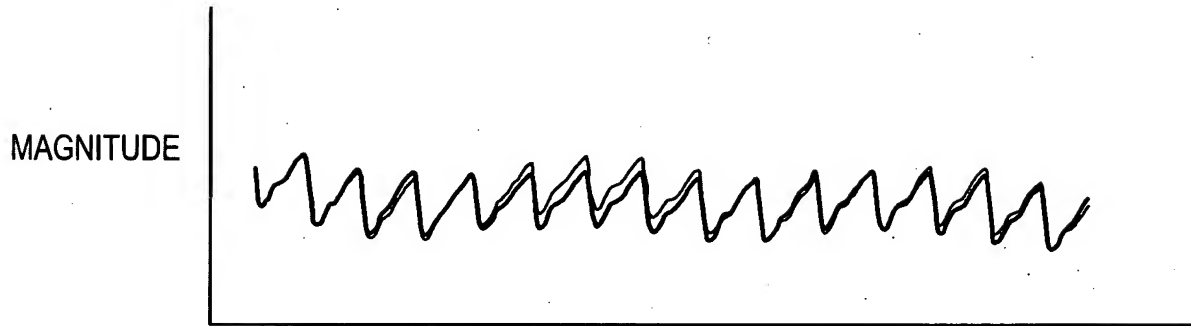

SAMPLE NUMBER

FIG.5A

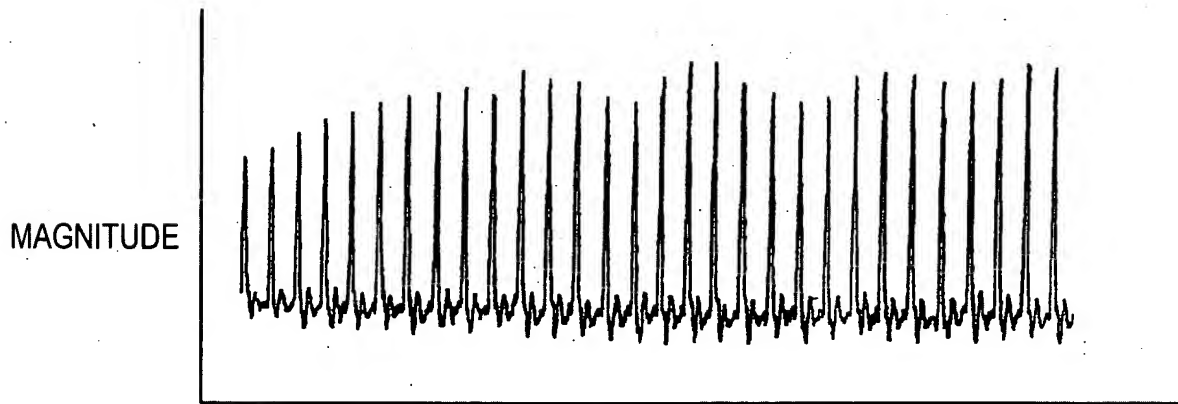

SAMPLE NUMBER

FIG.5B

10/19

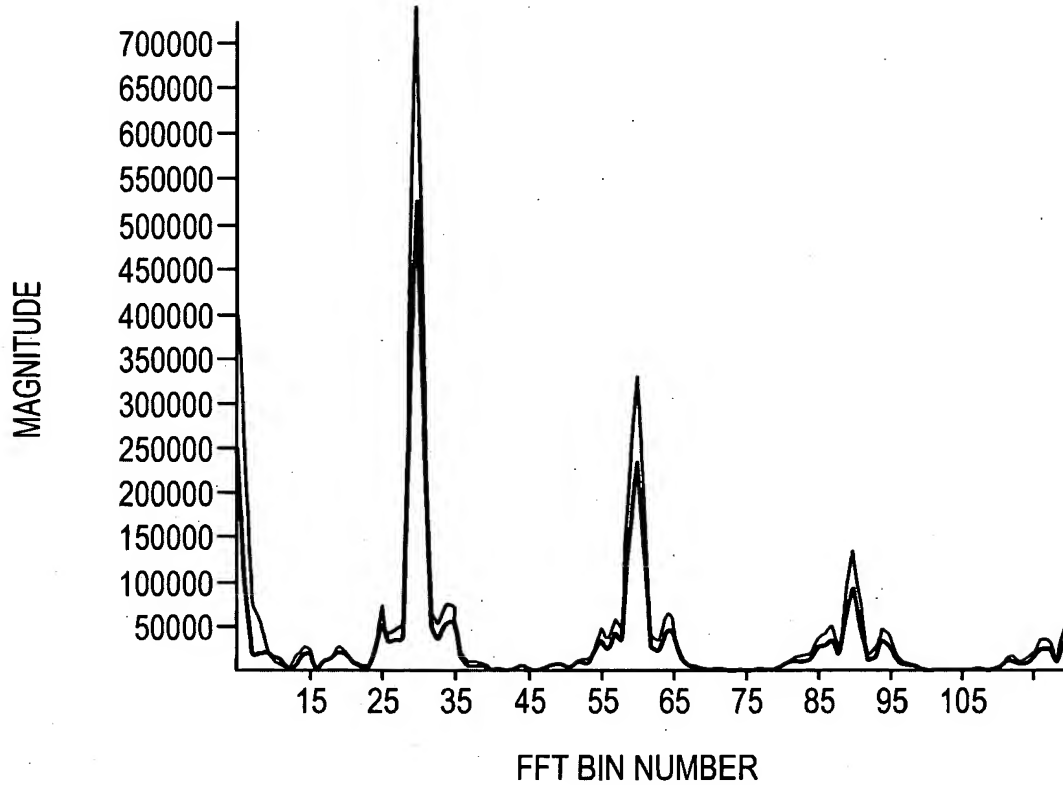


FIG.5C

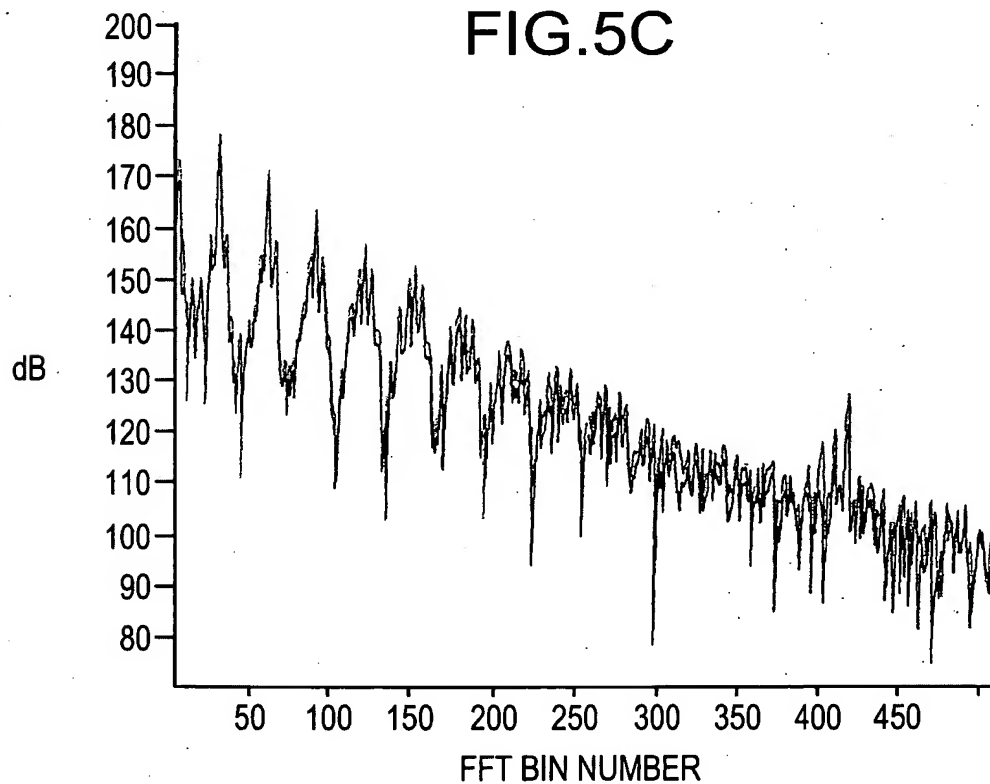


FIG.5D

11/19

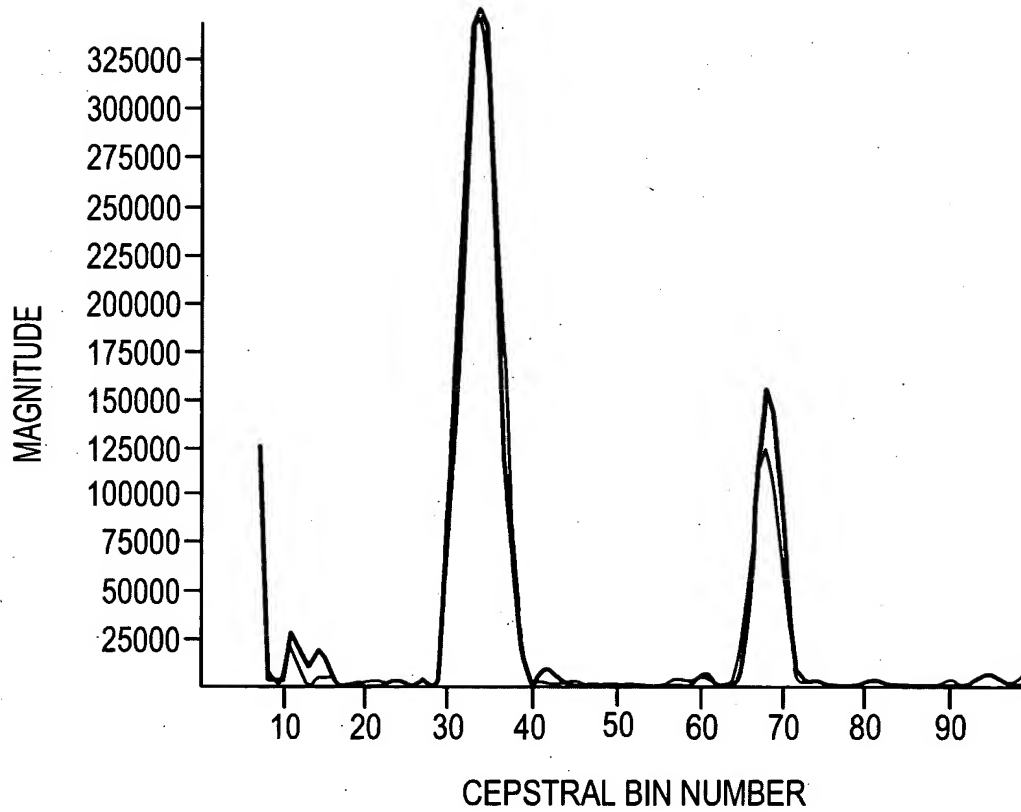


FIG.5E


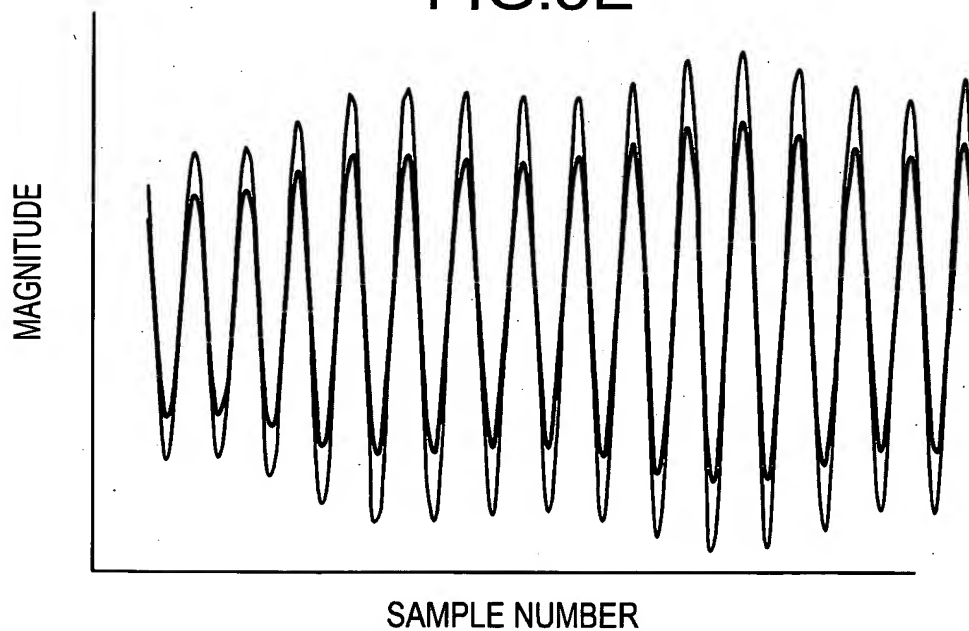


FIG.5F

12/19


MAGNITUDE

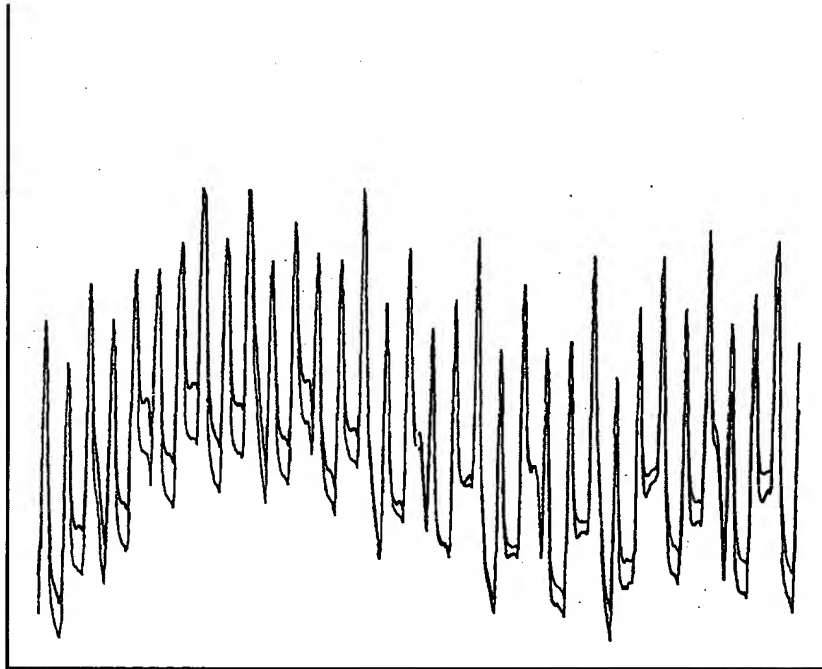

SAMPLE NUMBER

FIG.6A

MAGNITUDE

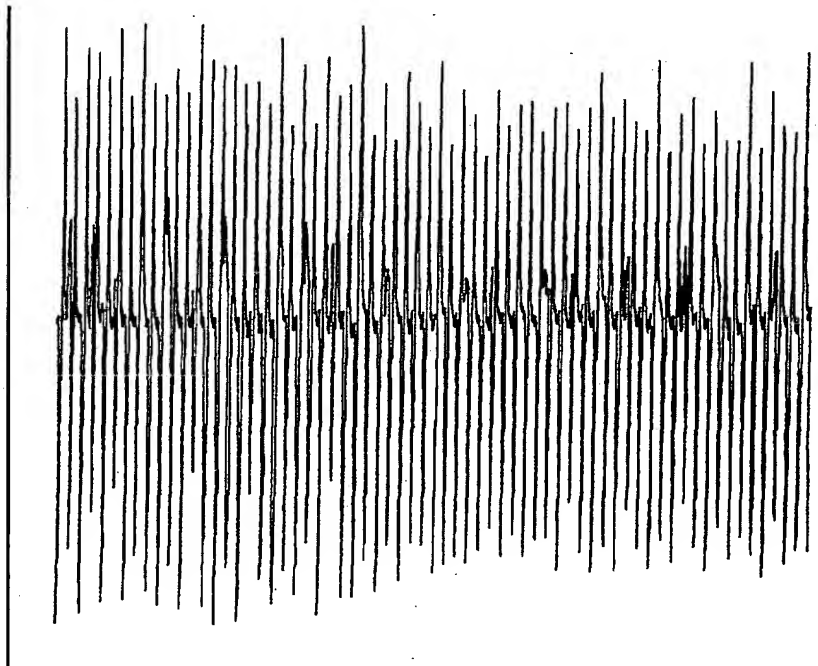

SAMPLE NUMBER

FIG.6B

13/19

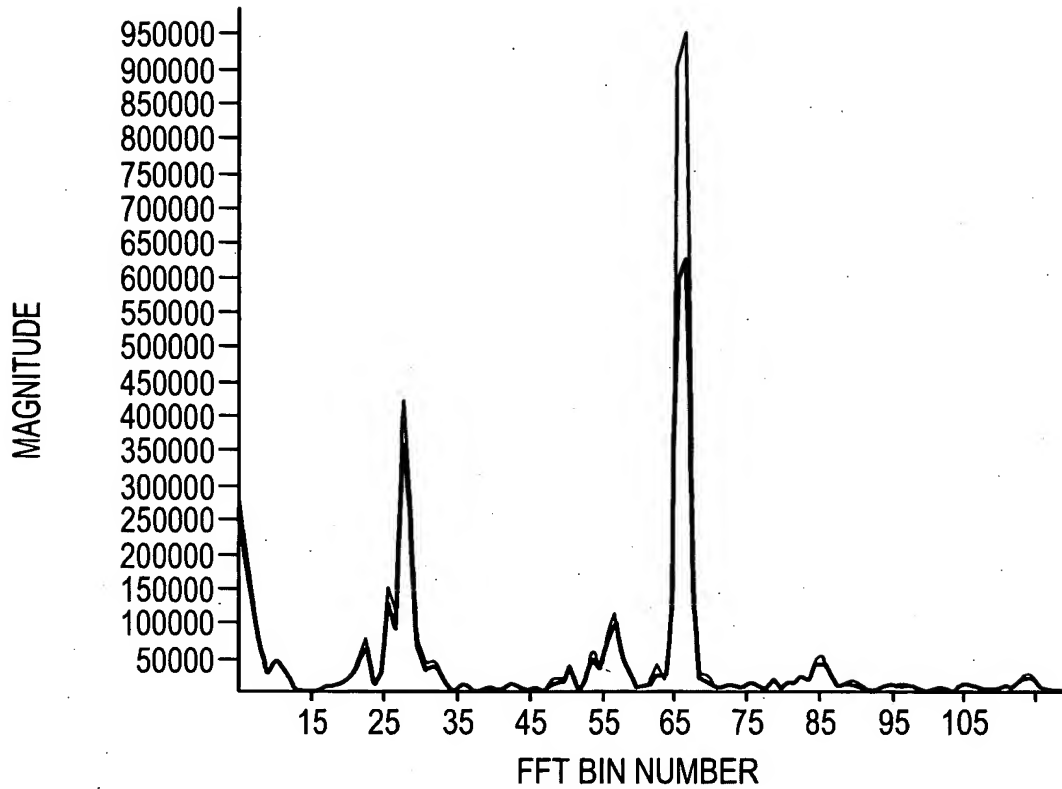


FIG. 6C

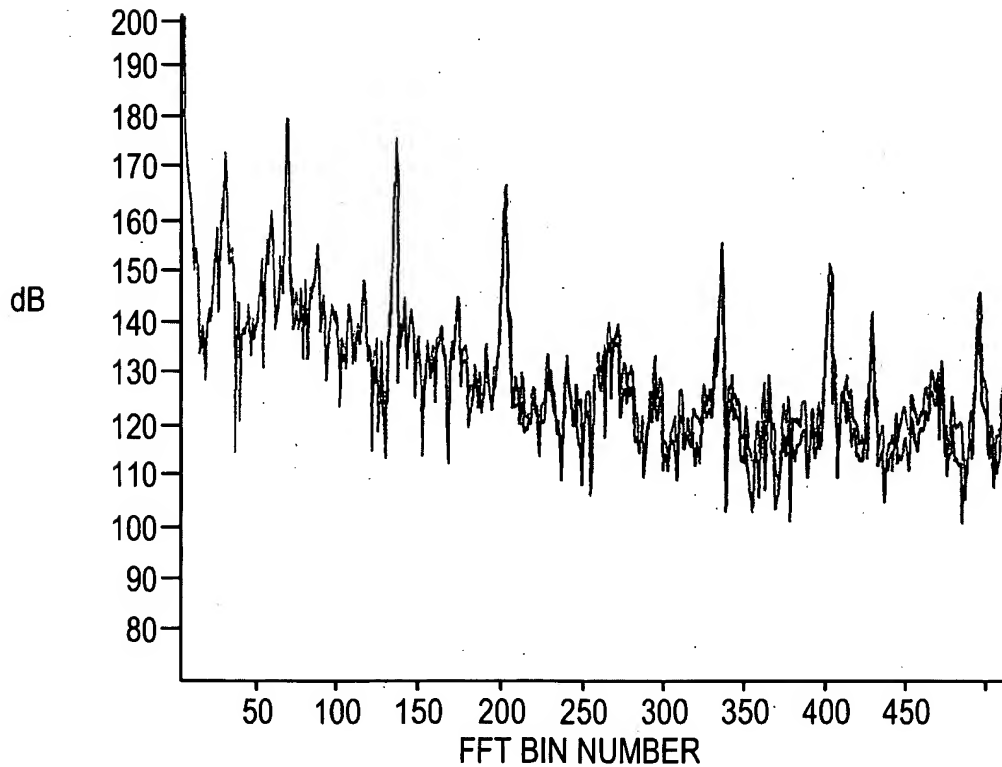


FIG. 6D

14/19

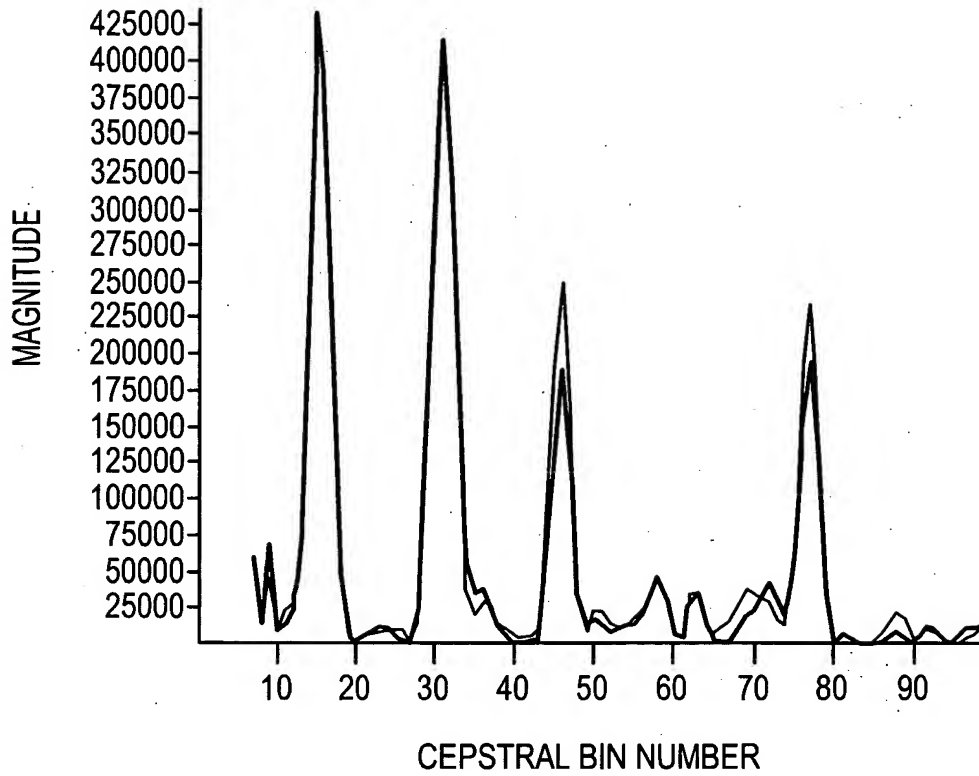


FIG.6E

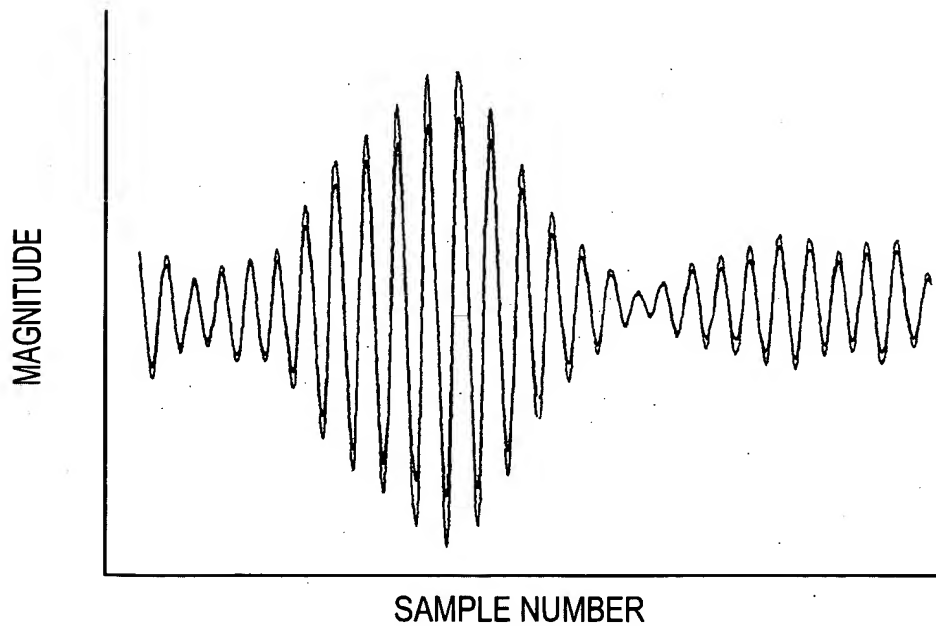


FIG.6F

15/19

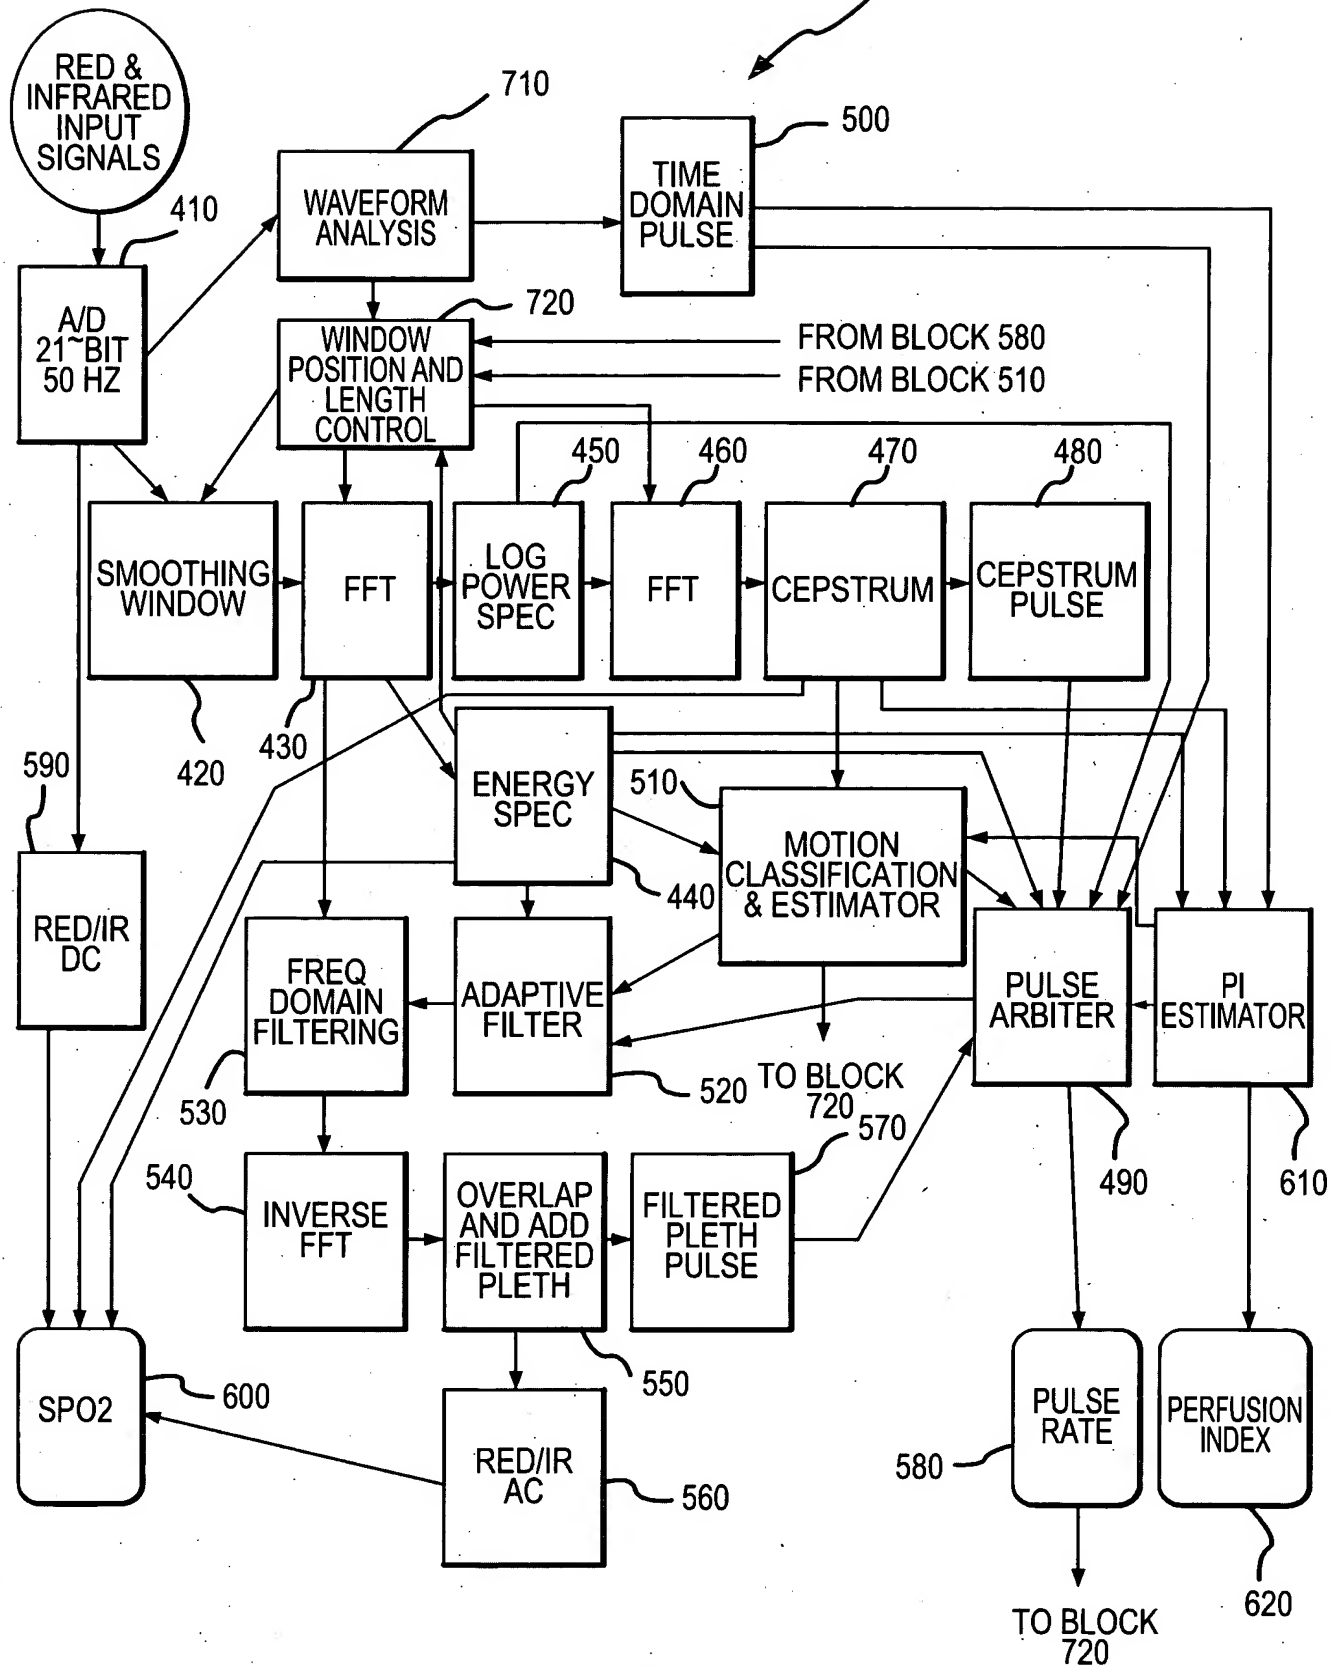


FIG.7

16/19

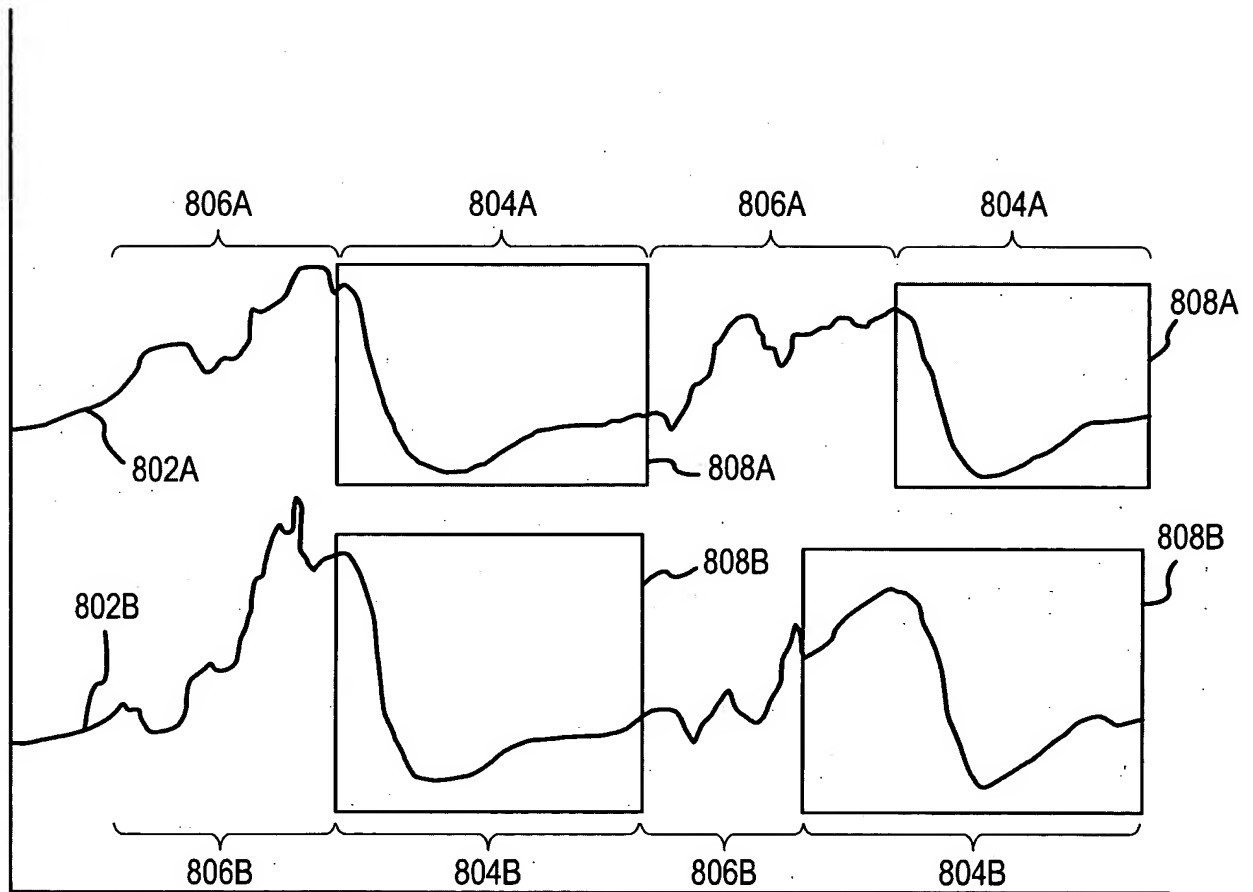


FIG.8

17/19

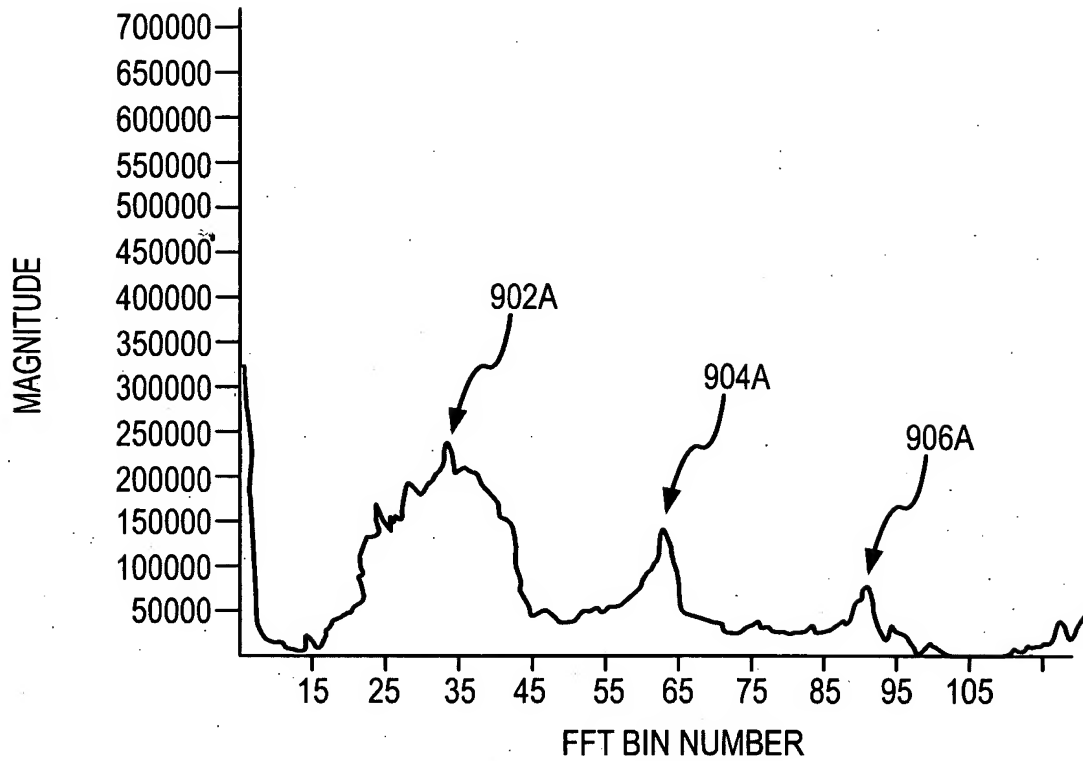


FIG. 9A

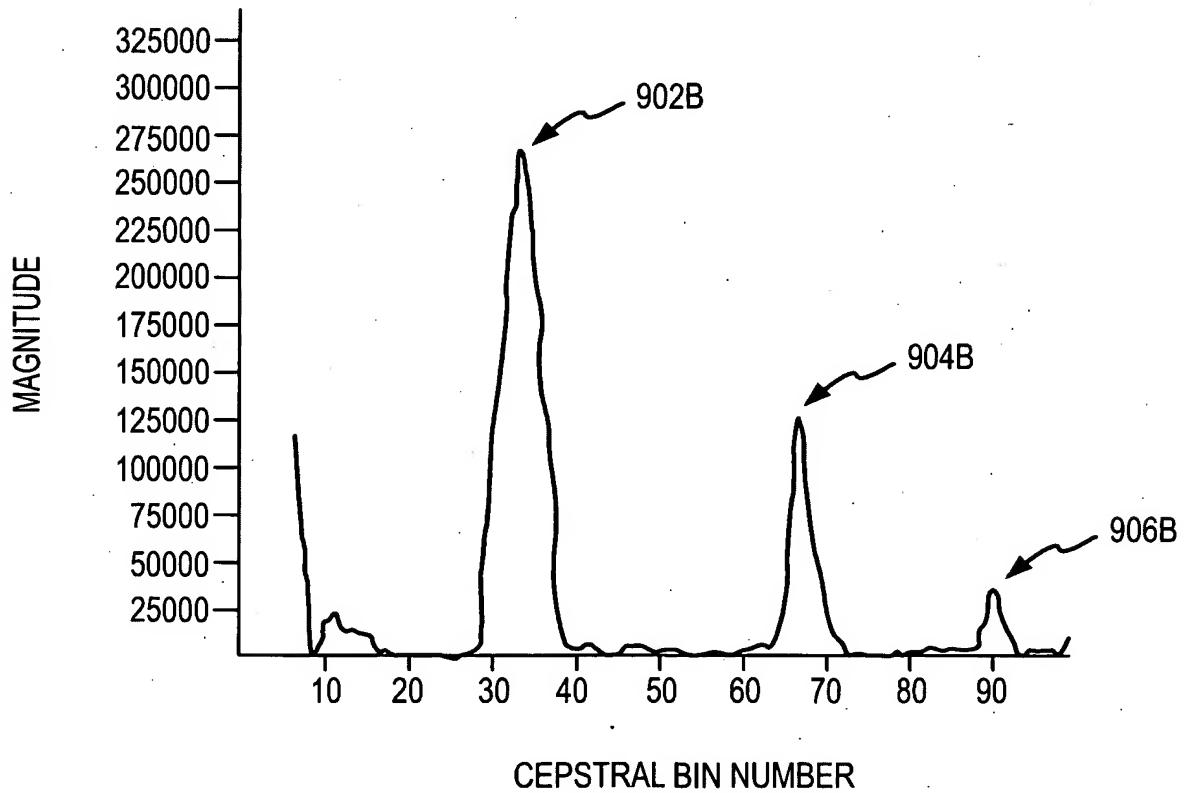


FIG. 9B

18/19

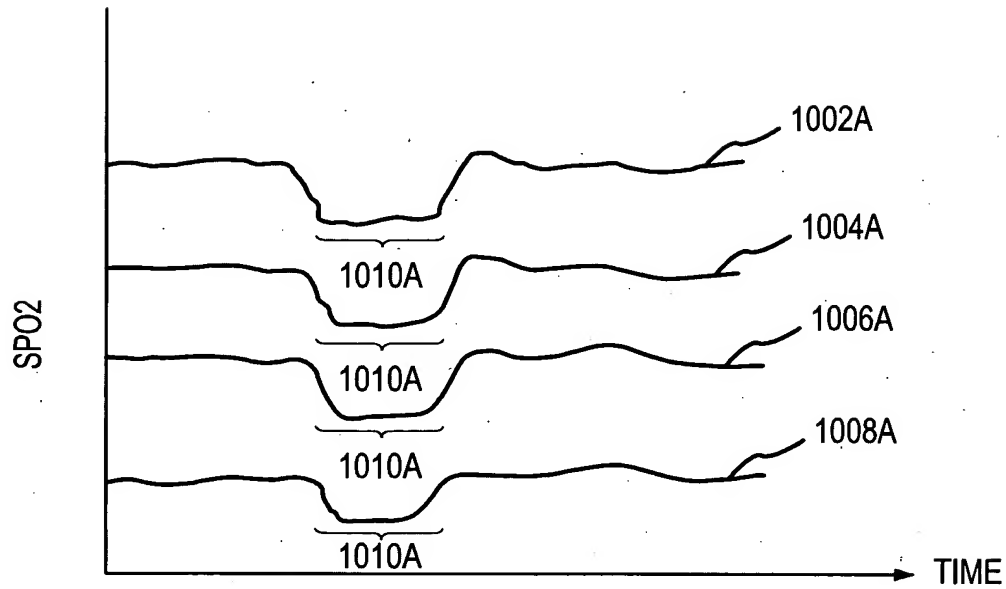


FIG.10A

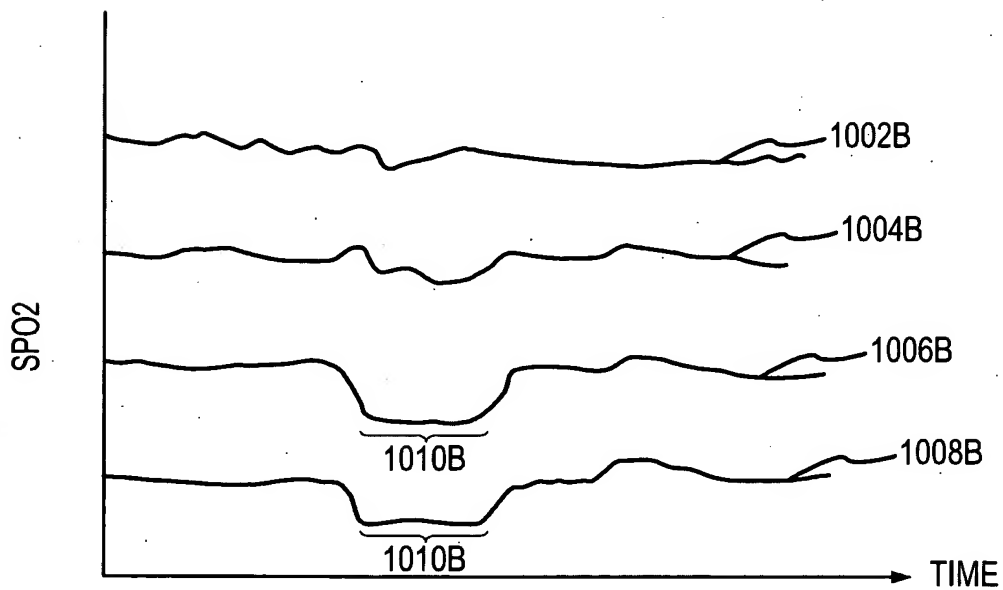


FIG.10B

19/19

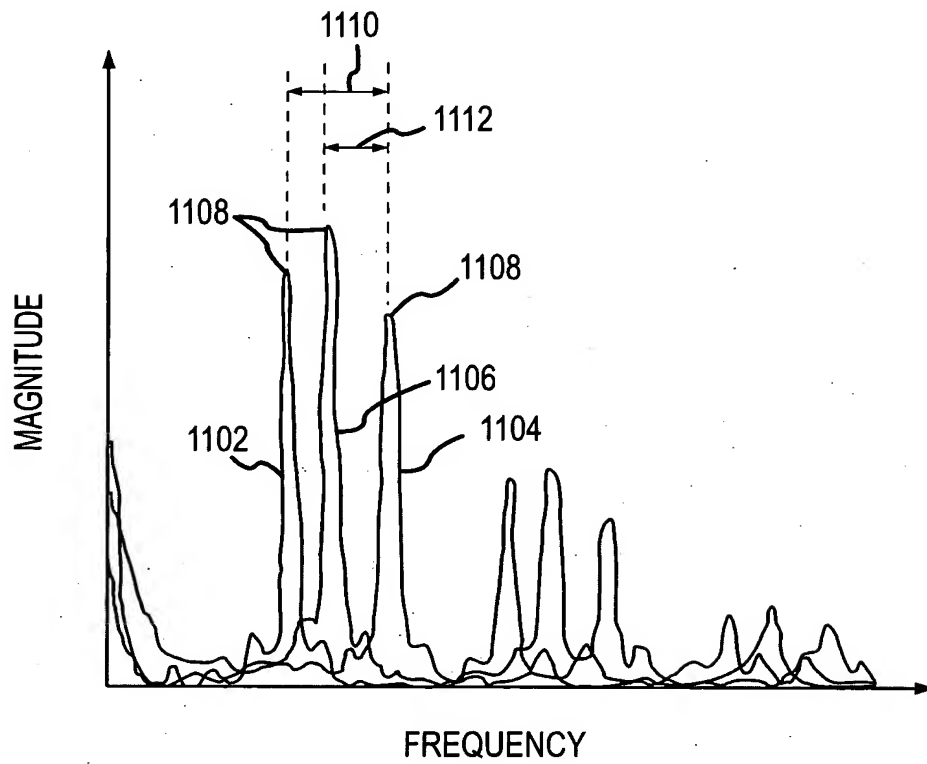


FIG. 11A

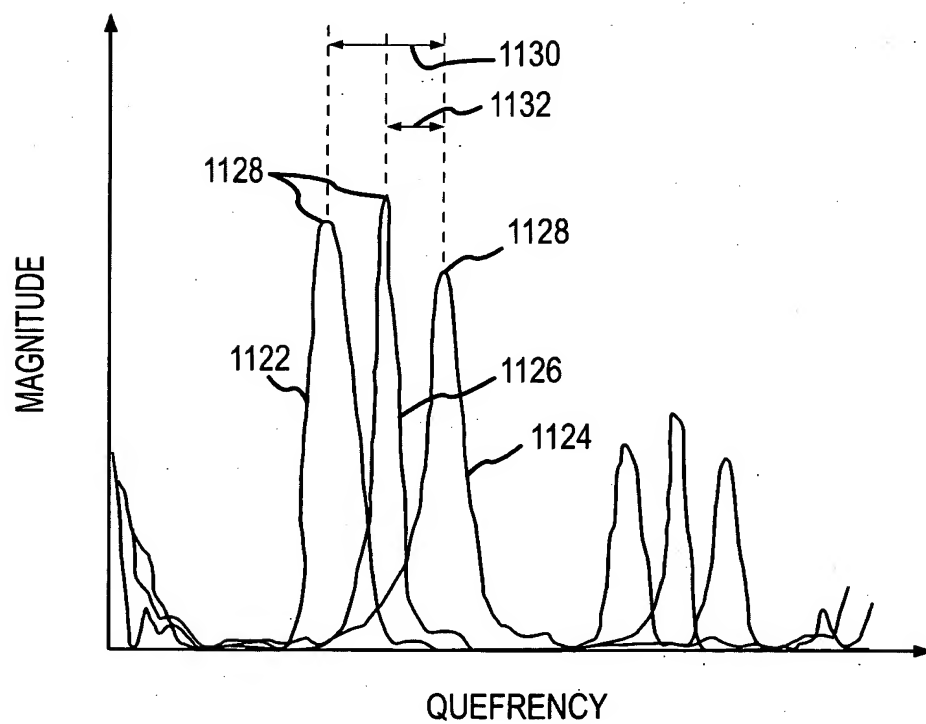


FIG. 11B